
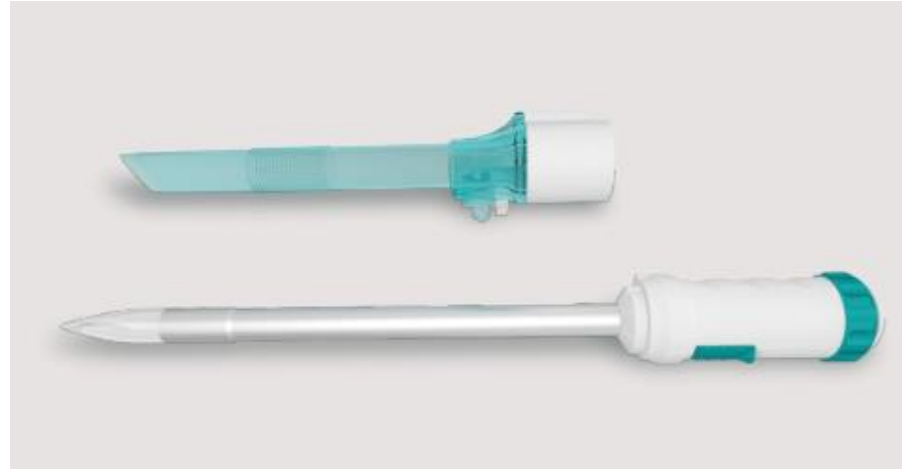
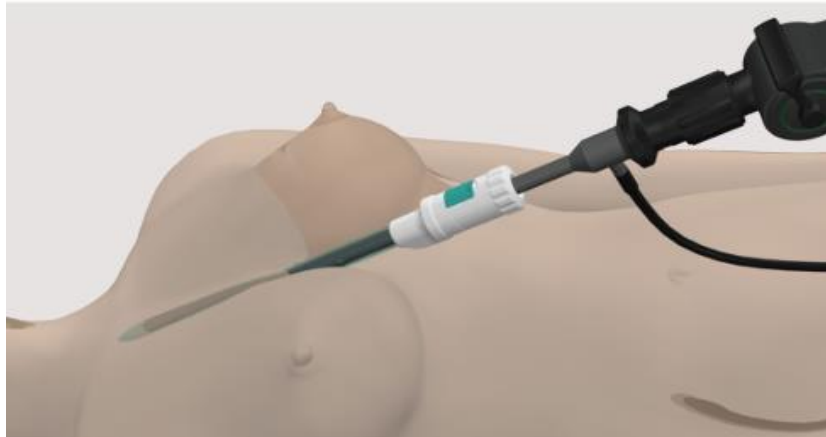
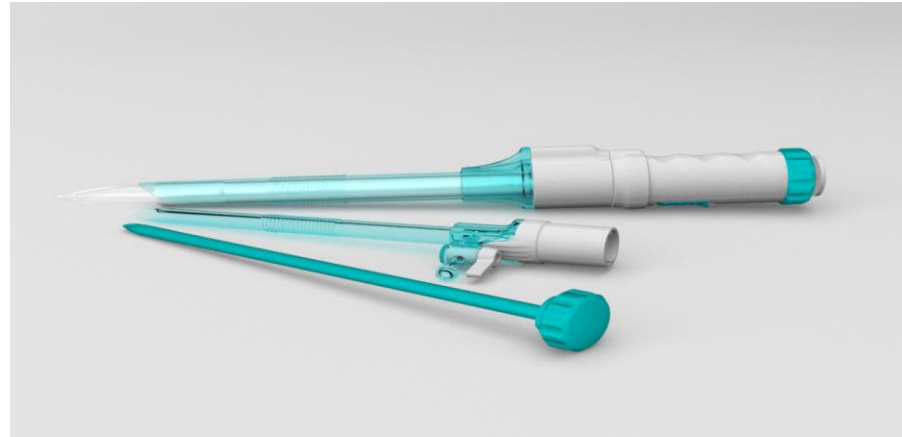


Disposable Thyroidectomy Trocar

Indications

Benign diseases such as simple goiter, nodular goiter (or with cystic hyperplasia), or thyroid adenoma

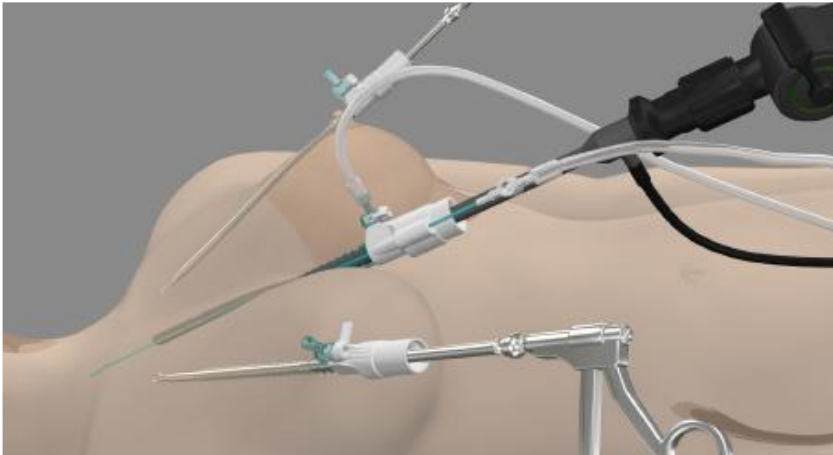

Disposable Thyroidectomy Trocar

Tip	Cannula	Obturator	Seal Style	Series	Length (mm)	Diameter (mm)
N Pyramid	P Threaded	C Non-Optical	S Single Sheet	A style	100 130	1-5 1-12 3-F(5/5/12)

No.	REF NO.	No.	REF NO.
1	NPCSA -130 -1-5	3	NPCSA-130-3-F
2	NPCSA -130 -1-12		